
Certificate of Analysis

Human NOS2/iNOS(Nitric oxide synthase, inducible) ELISA Kit

Cat.No.: MBS761262

Size: 96T


Lot:H0556C116

Principle: This ELISA kit use Sandwich-ELISA as the method

Product Performance Date: 20171121

This product has been tested by Quality Control Department and meets performance specifications mentioned in the manual.

| Concentration(pg/ml) | OD-1 | OD-2 | Average | OD-blank |
|----------------------|-------|-------|---------|----------|
| 0 | 0.097 | 0.101 | 0.099 | 0.000 |
| 78.125 | 0.139 | 0.145 | 0.142 | 0.043 |
| 156.25 | 0.204 | 0.212 | 0.208 | 0.109 |
| 312.5 | 0.356 | 0.370 | 0.363 | 0.264 |
| 625 | 0.693 | 0.721 | 0.707 | 0.608 |
| 1250 | 1.188 | 1.236 | 1.212 | 1.113 |
| 2500 | 1.816 | 1.890 | 1.853 | 1.754 |
| 5000 | 2.318 | 2.412 | 2.365 | 2.266 |

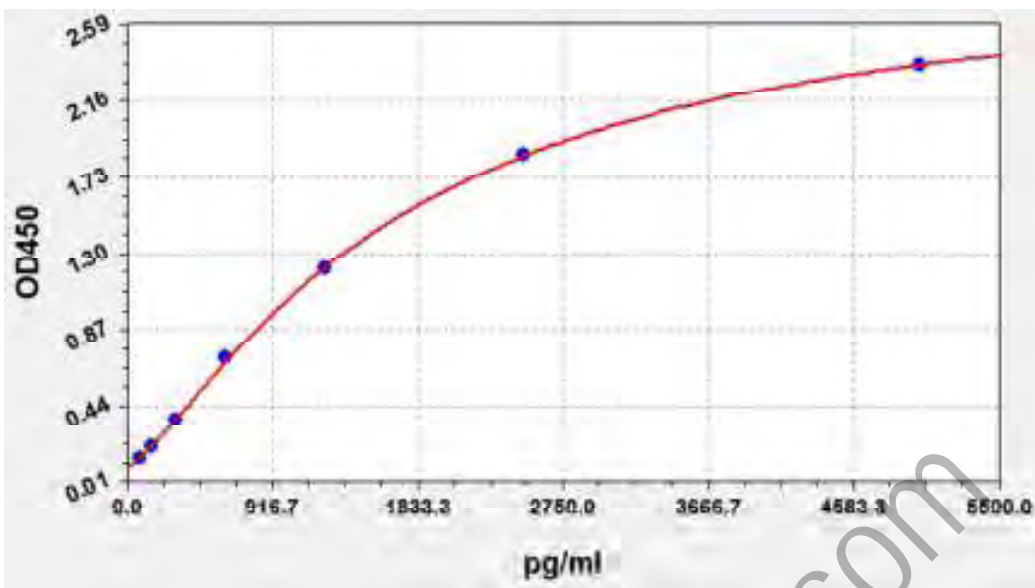

Performance Characteristics

Intra-Assay CV: $\leq 8\%$

Inter-Assay CV: $\leq 8\%$

Date: 2017/11/21