

# Certificate of Analysis

## Human LUM(Lumican) ELISA Kit

Cat.No.: **MBS763246**

Size:96T


Lot:H0220E044

**Principle:** This ELISA kit use Sandwich-ELISA as the method

**Product expiration Date:** 2019/10/15

This product has been tested by Quality Control Department and meets performance specifications mentioned in the manual.

Concentration(ng/ml)	OD-1	OD-2	Average	OD-blank
0	0.165	0.169	0.167	0.000
0.312	0.337	0.347	0.342	0.175
0.625	0.573	0.589	0.581	0.414
1.25	0.846	0.870	0.858	0.691
2.5	1.224	1.260	1.242	1.075
5	1.693	1.743	1.718	1.601
10	2.057	2.117	2.087	1.920
20	2.549	2.623	2.586	2.419

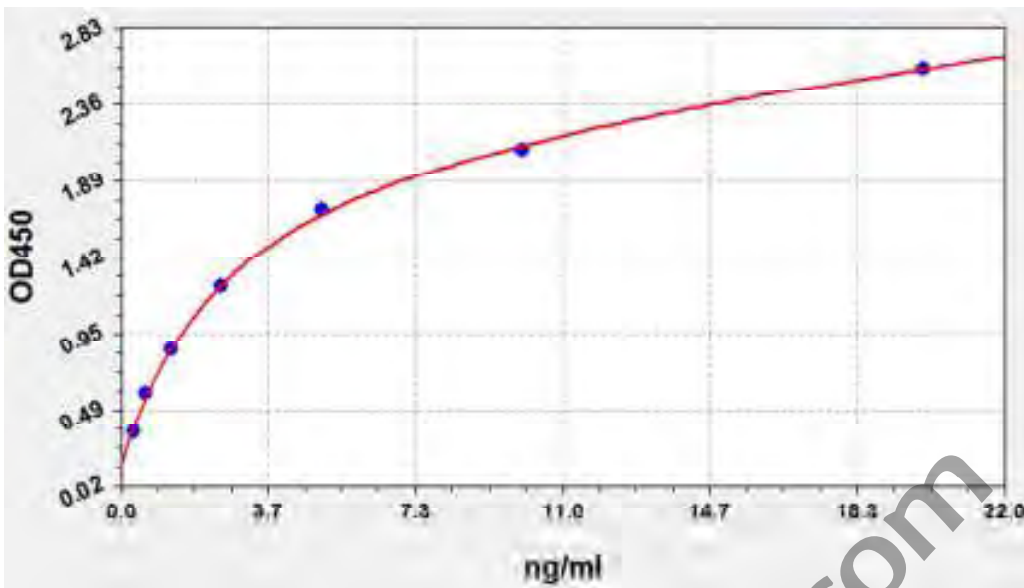

#### Performance Characteristics

Intra-Assay CV:  $\leq 8\%$

Inter-Assay CV:  $\leq 10\%$

Date: 2019/04/15