

Certificate of Analysis

PGE2(Prostaglandin E2) ELISA Kit

Cat.No.: **MBS763445**

Size: 96T


Lot:U2554E059

Principle: This ELISA kit uses Competitive-ELISA as the method

Product expiration Date: 2019/11/31

This product has been tested by Quality Control Department and meets performance specifications mentioned in the manual.

Concentration(pg/ml)	OD-1	OD-2	Average
0	2.286	2.352	2.319
31.25	1.676	1.724	1.7
62.5	1.443	1.485	1.464
125	1.059	1.089	1.074
250	0.709	0.729	0.719
500	0.548	0.564	0.556
1000	0.435	0.447	0.441
2000	0.277	0.285	0.281

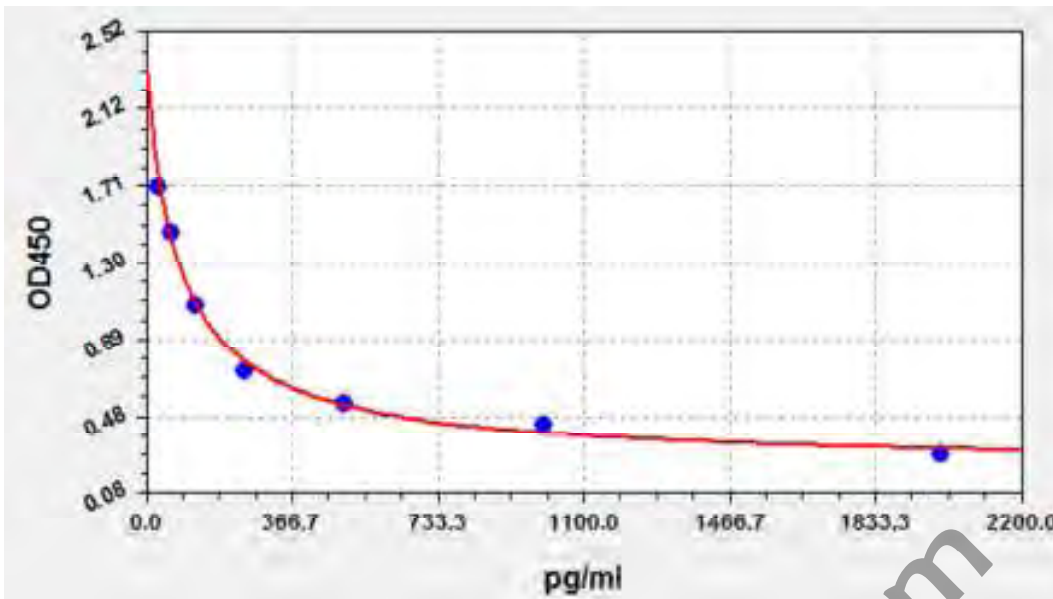

Performance Characteristics

Intra-Assay CV: $\leq 8\%$

Inter-Assay CV: $\leq 10\%$

Date: 2019/05/31