
Certificate of Analysis

Human PLK1(Serine/threonine-protein kinase PLK1) ELISA Kit

Cat.No.: MBS764924

Size: 96T


Lot: H1874D088

Principle: This ELISA kit uses Sandwich-ELISA as the method

Product expiration Date: 2019/02/27

This product has been tested by Quality Control Department and meets performance specifications mentioned in the manual.

Concentration(pg/ml)	OD-1	OD-2	Average	OD-blank
0	0.145	0.149	0.147	0.000
7.812	0.320	0.330	0.325	0.178
15.625	0.534	0.550	0.542	0.395
31.25	0.778	0.800	0.789	0.642
62.5	1.142	1.176	1.159	1.012
125	1.547	1.591	1.569	1.422
250	1.983	2.041	2.012	1.865
500	2.438	2.508	2.473	2.326

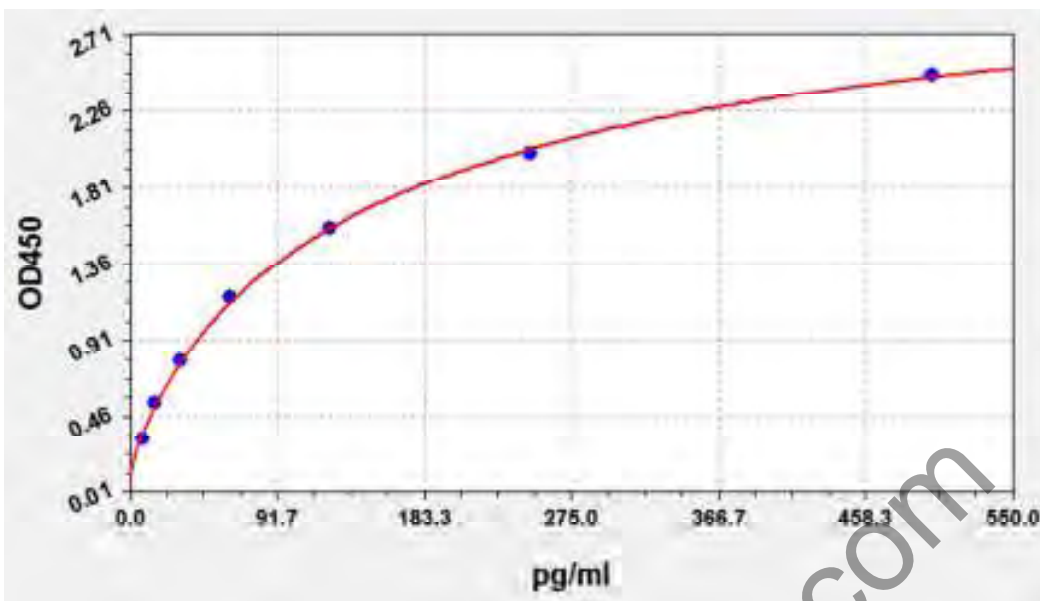

Performance Characteristics

Intra-Assay CV: $\leq 8\%$

Inter-Assay CV: $\leq 10\%$

Date: 2018/08/27