
Certificate of Analysis

Rat Epor(Erythropoietin receptor) ELISA Kit

Cat.No.: MBS765089

Size: 96T


Lot:R0223D073

Principle: This ELISA kit uses Sandwich-ELISA as the method

Product expiration Date: 2019/01/11

This product has been tested by Quality Control Department and meets performance specifications mentioned in the manual.

Concentration(ng/ml)	OD-1	OD-2	Average	OD-blank
0	0.078	0.080	0.079	0.000
0.156	0.173	0.179	0.176	0.097
0.312	0.301	0.309	0.305	0.226
0.625	0.587	0.605	0.596	0.517
1.25	1.158	1.192	1.175	1.096
2.5	1.975	2.033	2.004	1.925
5	2.834	2.916	2.875	2.796
10	3.527	3.629	3.578	3.499

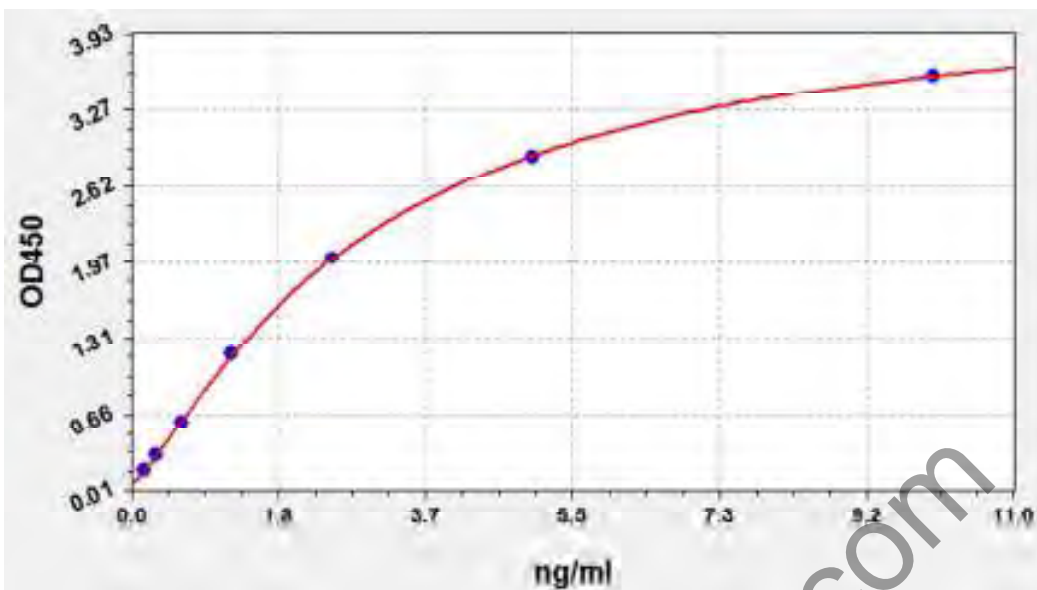

Performance Characteristics

Intra-Assay CV: $\leq 8\%$

Inter-Assay CV: $\leq 10\%$

Date: 2018/07/11