

Certificate of Analysis

Rat CD28(Cluster of Differentiation 28) ELISA Kit

Cat.No.: **MBS765774**

Size: 48T


Lot:R0814E079

Principle: This ELISA kit uses sandwich-ELISA as the method

Product expiration Date: 2020/01/30

This product has been tested by Quality Control Department and meets performance specifications mentioned in the manual.

Concentration(ng/ml)	OD-1	OD-2	Average	OD-blank
0	0.081	0.083	0.082	0.000
0.312	0.187	0.197	0.192	0.110
0.625	0.191	0.201	0.196	0.114
1.25	0.289	0.275	0.282	0.200
2.5	0.470	0.484	0.477	0.395
5	0.876	0.920	0.898	0.816
10	1.422	1.388	1.405	1.323
20	2.297	2.411	2.354	2.272

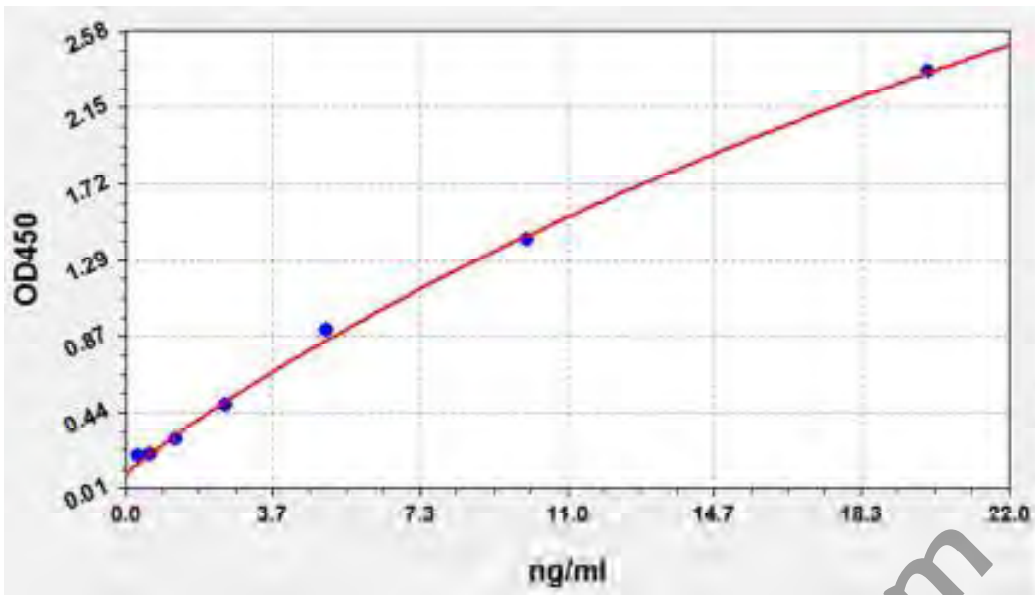

Performance Characteristics

Intra-Assay CV: $\leq 8\%$

Inter-Assay CV: $\leq 10\%$

Authorization

Released by: Lin Ze

Date: 2019/07/30