

Certificate of Analysis

PRODUCT INFORMATION

Catalog Number: MBS8241404


Product Name: siRNA Negative Control


Lot Number: GL2A02B

siRNA Negative Control:

Sequence: UUCUCCGAACGUGUCACGUTT
ACGUGACACGUUCGGAGAATT

QC Data:

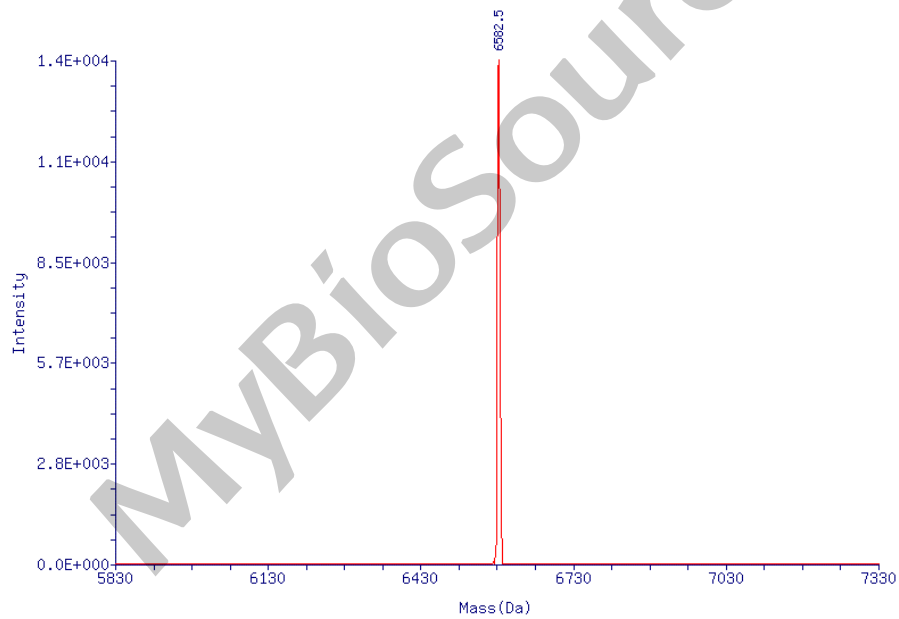

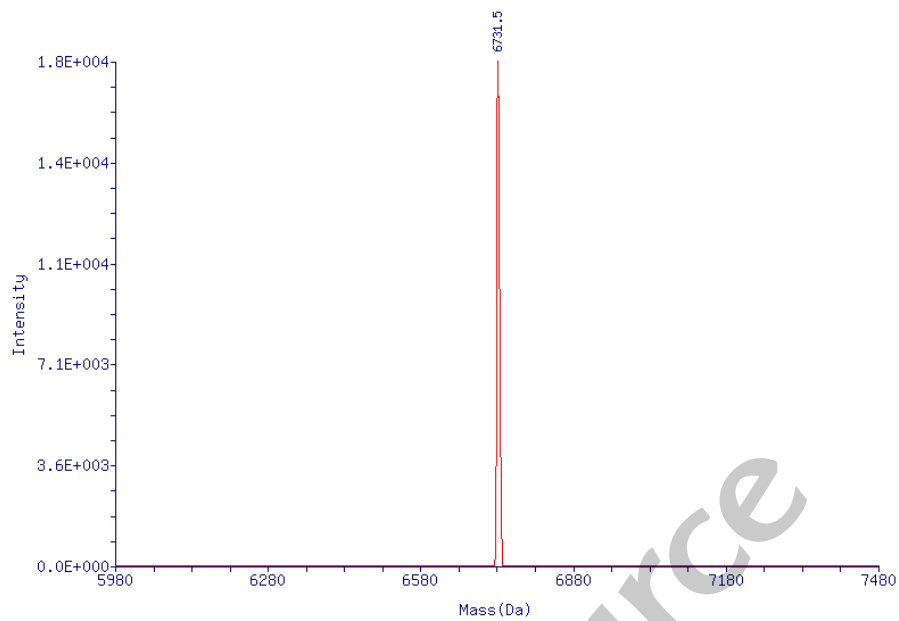

Equipment

LTQ Mass Spectrometer

QC standard

The difference between the actual and the theoretical molecular weight is less than 0.3%.

QC Result

Pass