

## **Human Leptin ELISA KIT**

### **Human Leptin ELISA KIT**

**Catalog Number**

MBS8506134

### **Human Leptin ELISA KIT**

For the quantitative determination of human Leptin concentrations in cell culture supernates, serum, and plasma. This package insert must be read in its entirety before using this product. If you have questions or experience problems with this product, please contact our Technical Support staff. Our scientists commit themselves to providing rapid and effective help.

**FOR RESEARCH USE ONLY  
NOT FOR USE IN DIAGNOSTIC PROCEDURES**

**For Research Use Only**

## INTRODUCTION


Human Leptin (gene name OB) is a 16 kDa, 146 amino acid (aa) residue, non-glycosylated polypeptide that regulates adipose tissue mass and energy balance (1 - 6). Mature human Leptin shares 87% and 84% aa identity with mouse and rat Leptin, respectively (1,7). Human Leptin is active in both the mouse and rat systems (8, 9). Leptin is expressed almost exclusively by adipocytes and its production is influenced by hormones, cytokines and nutrients (5, 7, 10) and circulates in the plasma, crosses the blood-brain barrier, and is present in human breast milk (3 - 6, 11). The human Leptin receptor (designated ObR or LEPR) is a 150 kDa, 1144 aa residue, type I transmembrane glycoprotein of the IL-6 receptor family of Class I cytokine receptors (12, 13). The gene for ObR undergoes considerable splicing, forming variants a-d with cytoplasmic domains of variable length, plus the potentially soluble form ObRe (13, 14). The long form, ObRb (formerly OB RL), is expressed mainly in the hypothalamic arcuate nucleus and is essential for signal transduction (6, 15, 16). In a concentration-dependent manner, Leptin signaling can have diverse effects, causing neurons that express pro-opiomelanocortin (POMC) peptides to reduce food intake, and neurons that express neuropeptide Y and agouti-related protein (NpY and AgRP) to increase food intake (4, 6). Leptin is fundamentally a "starvation signal" that, when low, prompts increased appetite and decreased energy expenditure (4, 6, 10). Leptin deficiency influences the immune system, depressing Th1 responses and causing increased frequency of infections (4). Leptin also regulates puberty, blocking the onset of puberty, or of menses if Leptin deficiency exists due to excessive thinness, such as results from starvation, extreme exercise-induced weight loss, anorexia or cancer-induced cachexia (3, 4).

## PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. A monoclonal antibody specific for Leptin has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any Leptin present is bound by the immobilized antibody. Following incubation unbound samples are removed during a wash step, and then a detection antibody specific for Leptin is added to the wells and binds to the combination of capture antibody- Leptin in sample. Following a wash to remove any unbound combination, and enzyme conjugate is added to the wells. Following incubation and wash steps a substrate is added. A coloured product is formed in proportion to the amount of Leptin present in the sample. The reaction is terminated by addition of acid and absorbance

**For Research Use Only**

is measured at 450nm. A standard curve is prepared from seven Leptin standard dilutions and Leptin sample concentration determined.

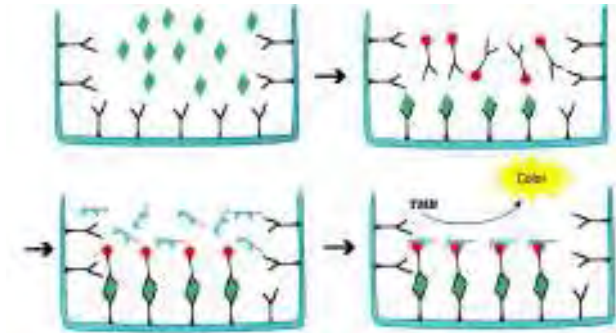

**Figure 1: Schematic diagram of the assay**

## REAGENTS

1. Aluminium pouches with a Microwell Plate coated with antibody to human Leptin (8x12)
2. 2 vials human Leptin Standard lyophilized, 2000 pg/ml upon reconstitution
3. 2 vials concentrated Biotin-Conjugate anti-human Leptin antibody
4. 2 vials Streptavidin-HRP solution
5. 4 bottle Standard /sample Diluent
6. 1 bottle Biotin-Conjugate antibody Diluent
7. 1 bottle Streptavidin-HRP Diluent
8. 1 bottle Wash Buffer Concentrate 20x (PBS with 1% Tween-20)
9. 1 vial Substrate Solution
10. 1 vial Stop Solution
11. 4 pieces Adhesive Films
12. package insert

**NOTE:** [96 Tests]

## STORAGE

Table 1: Storage of the kit

**For Research Use Only**

<b>Unopened Kit</b>	Store at 2 – 8°C. Do not use past kit expiration date.	
<b>Opened/ Reconstituted Reagents</b>	Standard /sample Diluent	May be stored for up to 1 month at 2 – 8°C. **
	Concentrated Biotin-Conjugate	
	Streptavidin-HRP solution	
	Biotin-Conjugate antibody Diluent	
	Streptavidin-HRP Diluent	
	Wash Buffer Concentrate 20x	
	Substrate Solution	
	Stop Solution	
	Standard	Aliquot and store for up to 1 month at ≤20°C. Avoid repeated freeze-thaw cycles. Diluted standard shall not be reused.
	Microplate Wells	Return unused wells to the foil pouch containing the desiccant pack, reseal along entire edge of zip-seal. May be stored for up to 1 month at 2 – 8°C. **

\*\*Provided this is within the expiration date of the kit.

### THE REQUIRED ITEMS (not provided, but can help to buy)

1. Microplate reader (450nm).
2. Micro-pipette and tips: 0.5-10, 2-20, 20-200, 200-1000µl.
3. 37 °C incubator, double-distilled water or deionized water, coordinate paper, graduated cylinder.

### PRECAUTIONS FOR USE

1. Store kit reagents between 2°C and 8°C. After use all reagents should be immediately returned to cold storage (2°C to 8°C).
2. Please perform simple centrifugation to collect the liquid before use.
3. To avoid cross contamination, please use disposable pipette tips.
4. The Stop Solution suggested for use with this kit is an acid solution. Wear eye, hand, face, and clothing protection when using this material.

**For Research Use Only**

Avoid contact of skin or mucous membranes with kit reagents or specimens. In the case of contact with skin or eyes wash immediately with water.

5. Use clean, dedicated reagent trays for dispensing the washing liquid, conjugate and substrate reagent. Mix all reagents and samples well before use.
6. After washing microtiter plate should be fully pat dried. Do not use absorbent paper directly into the enzyme reaction wells.
7. Do not mix or substitute reagents with those from other lots or other sources. Do not use kit reagents beyond expiration date on label.
8. Each sample, standard, blank and optional control samples should be assayed in duplicate or triplicate.
9. Adequate mixing is very important for good result. Use a mini-vortexer at the lowest frequency or Shake by hand at 10min interval when there is no vortexer.
10. Avoid microtiter plates drying during the operation.
11. Dilute samples at the appropriate multiple, and make the sample values fall within the standard curve. If samples generate values higher than the highest standard, dilute the samples and repeat the assay.
12. Any variation in standard diluent, operator, pipetting technique, washing technique, incubation time and temperature, and kit age can cause variation in binding.
13. This method can effectively eliminate the interference of the soluble receptors, binding proteins and other factors in biological samples.

## **SAMPLE COLLECTION AND STORAGE**

1. **Cell Culture Supernates** - Remove particulates by centrifugation.
2. **Serum** - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at approximately 1000 x g. Remove serum, avoid hemolysis and high blood lipid samples.
3. **Plasma** - Recommended EDTA as an anticoagulant in plasma. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection.
4. Assay immediately or aliquot and store samples at -20°C. Avoid repeated freeze-thaw cycles.
5. Dilute samples at the appropriate multiple (recommended to do pre-test

**For Research Use Only**

to determine the dilution factor).

**Note: The normal human serum or plasma samples are suggested to make a 1:10 dilution.**

## REAGENT PREPARATION

1. Bring all reagents to room temperature before use.
2. **Wash Buffer** - Dilute 10ml of Wash Buffer Concentrate into deionized or distilled water to prepare 200ml of Wash Buffer. If crystals have formed in the concentrate Wash Buffer, warm to room temperature and mix gently until the crystals have completely dissolved.
3. **Standard** - Reconstitute the Standard with 1.0ml of Standard /sample Diluent. This reconstitution produces a stock solution of 2000 pg /mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions.

Pipette 500µl of Standard/sample Diluent into the 1000 pg/ml tube and the remaining tubes. Use the stock solution to produce a 2-fold dilution series (below). Mix each tube thoroughly and change pipette tips between each transfer. The 2000 pg/ml standard serves as the high standard. The Standard/ sample Diluent serves as the zero standard (0 pg/ml).

**If you do not run out of re-melting standard, store it at -20°. Diluted standard shall not be reused.**


4. Working solution of Biotin-Conjugate anti-human Leptin antibody: Make a 1:100 dilution of the concentrated Biotin-Conjugate solution with the Biotin-Conjugate antibody Diluent in a clean plastic tube.

**The working solution should be used within one day after dilution.**

5. Working solution of Streptavidin-HRP: Make a 1:100 dilution of the concentrated Streptavidin-HRP solution with the Streptavidin-HRP Diluent in a clean plastic tube.

**The working solution should be used within one day after dilution.**

**For Research Use Only**

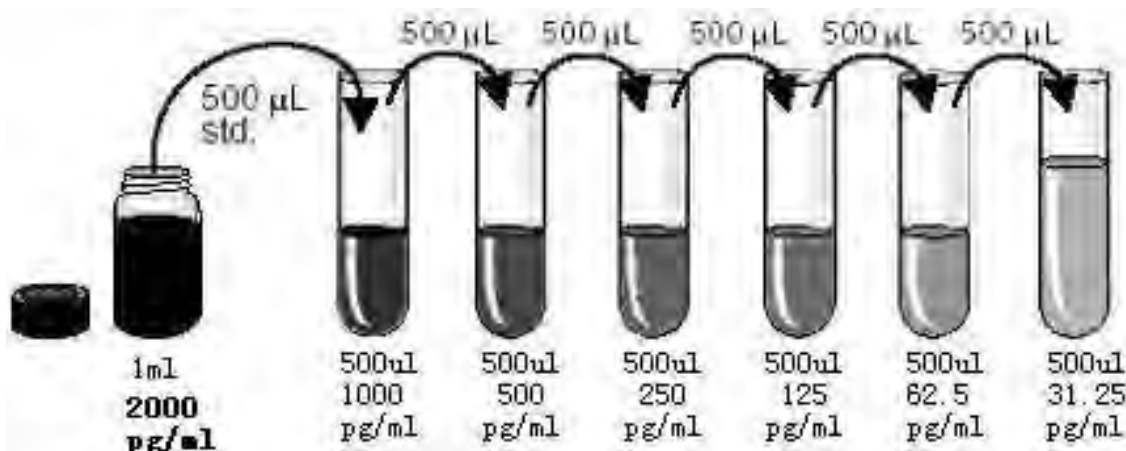

**Figure 2: Preparation of Leptin standard dilutions**

## GENERAL ELISA PROTOCOL

1. Prepare all reagents and working standards as directed in the previous sections.
2. Determine the number of microwell strips required to test the desired number of samples plus appropriate number of wells needed for running blanks and standards. Remove extra microwell strips from holder and store in foil bag with the desiccant provided at 2-8 °C sealed tightly.
3. Add 100 µL of Standard, control, or sample, per well. Cover with the adhesive strip provided. Incubate for 1.5 hours at 37 °C.
4. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with Wash Buffer (350 µL) using a squirt bottle, manifold dispenser or auto-washer. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
5. Add 100 µL of the working solution of Biotin-Conjugate to each well. Cover with a new adhesive strip and incubate 1 hour at 37 °C.
6. Repeat the aspiration/wash as in step 4.
7. Add 100 µL of the working solution of Streptavidin-HRP to each well. Cover with a new adhesive strip and incubate for 30 minutes at 37 °C. Avoid placing the plate in direct light.

**For Research Use Only**

8. Repeat the aspiration/wash as in step 4.
9. Add 100µl of Substrate Solution to each well. Incubate for 10-20 minutes at 37°C. Avoid placing the plate in direct light.
10. Add 100µl of Stop Solution to each well. Gently tap the plate to ensure thorough mixing.
11. Determine the optical density of each well immediately, using a microplate reader set to 450 nm.(optionally 650nm as the reference wave length;610-650nm is acceptable)

MyBioSource.com

**For Research Use Only**



## ASSAY PROCEDURE SUMMARY

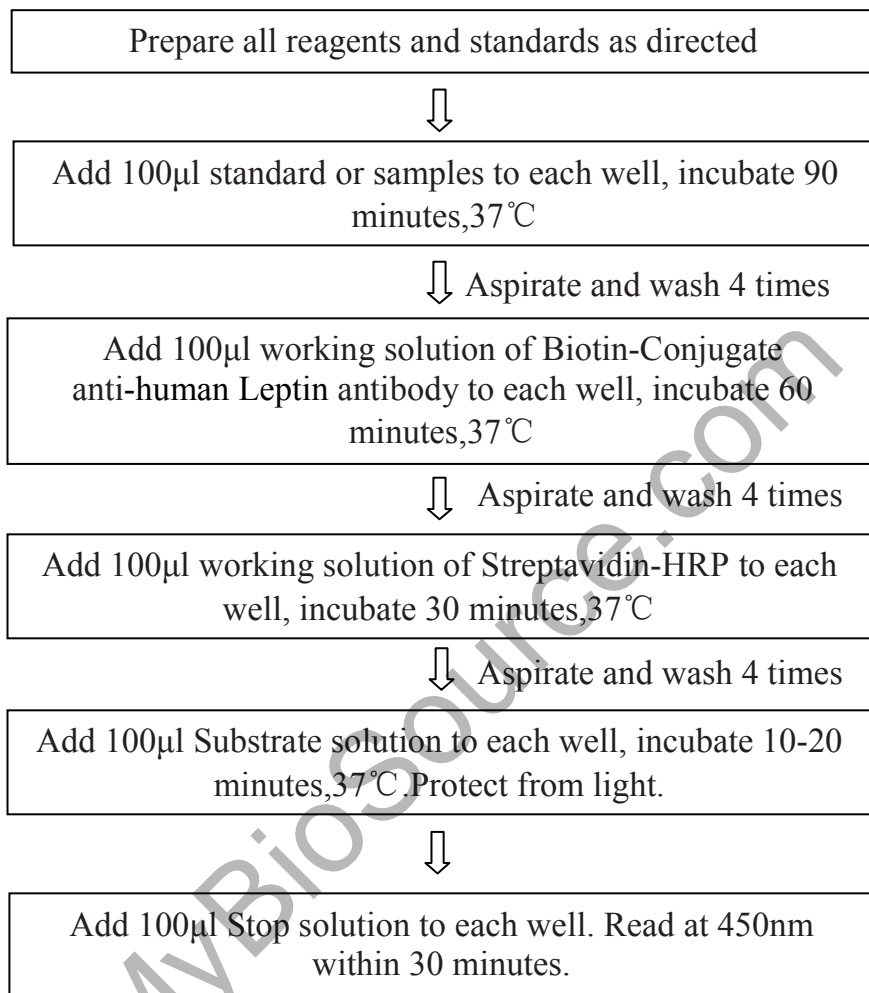


Figure 3: Assay procedure summary

## TECHNICAL HINTS

1. When mixing or reconstituting protein solutions, always avoid foaming.
2. To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.
3. To ensure accurate results, proper adhesion of plate sealers during incubation steps is necessary.

**For Research Use Only**

4. Substrate Solution should remain colorless until added to the plate. Stop Solution should be added to the plate in the same order as the Substrate Solution. Keep Substrate Solution protected from light. Substrate Solution should change from colorless to gradations of blue.
5. A standard curve should be generated for each set of samples assayed. According to the content of tested factors in the sample, appropriate diluted or concentrated samples, it is best to do pre-experiment.

## **CALCULATION OF RESULTS**

1. Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density.
2. Create a standard curve by reducing the data using computer software capable of generating a four parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph.
3. The data may be linearized by plotting the log of the Leptin concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.
4. This standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

Table 2: Typical data using the Leptin ELISA (Measuring wavelength: 450nm, Reference wavelength: 650nm)

**For Research Use Only**

Standard (pg/ml)	OD.	OD.	Average	Corrected
0	0.058	0.056	0.057	—
31.25	0.065	0.067	0.066	0.038
62.5	0.083	0.089	0.086	0.084
125	0.135	0.135	0.135	0.175
250	0.278	0.280	0.279	0.352
500	0.650	0.664	0.657	0.691
1000	1.371	1.360	1.365	1.301
2000	2.251	2.232	2.241	2.254

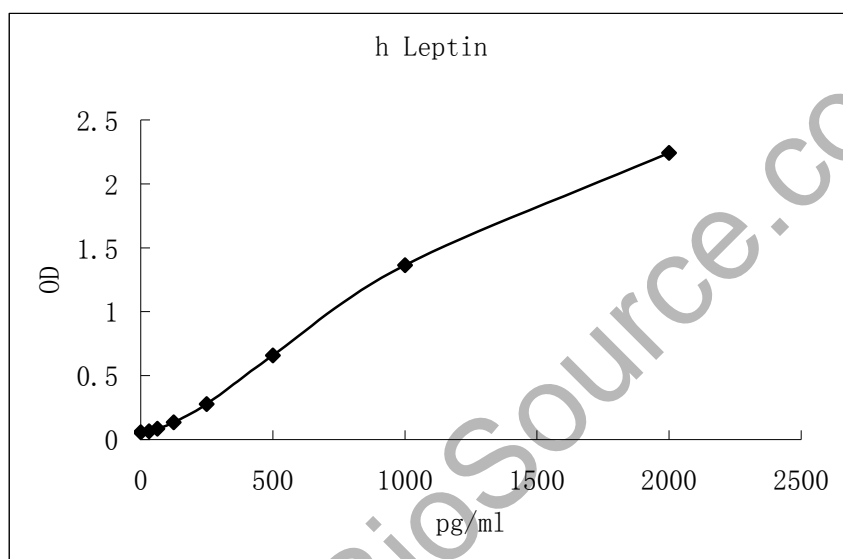


Figure 4: Representative standard curve for Leptin ELISA. Leptin was diluted in serial two-fold steps in Sample Diluent.

**Do not use this standard curve to derive test results. A standard curve must be run for each group of microwell strips assayed.**

### SENSITIVITY, SPECIFICITY AND REPEATABILITY

1. **REPEATABILITY:** The coefficient of variation of both intra-assay and inter-assay were less than 10%.
2. **SENSITIVITY:** The minimum detectable dose was 7pg/mL.
3. **SPECIFICITY:** This assay recognizes both natural and recombinant human Leptin. The factors listed below were prepared at 50ng/ml in

**For Research Use Only**

Standard /sample Diluent and assayed for cross-reactivity and no significant cross-reactivity or interference was observed.

Table 3: Factors assayed for cross-reactivity

Recombinant human	Recombinant mouse	Other proteins
G-CSF	Leptin	bovine FGF acidic
GM-CSF	LIF	bovine FGF basic
IL-1 $\alpha$	MIP-1 $\alpha$	human PDGF
IL-1 $\beta$	MIP-1 $\beta$	porcine PDGF
IL-2	TNF- $\alpha$	human TGF- $\beta$ 1
IL-3	IL-1 $\alpha$	porcine TGF- $\beta$ 1
IL-4	IL-1 $\beta$	porcine TGF- $\beta$ 2
	IL-3	

## REFERENCES

1. Zhang, Y. et al. (1994) Nature 372:425.
2. Cohen, S.L. et al. (1996) Nature 382:589.
3. Friedman, J.M. (2009) Am. J. Clin. Nutr. 89:973S.
4. Farooqi, I.S. and S. O'Rahilly (2009) Am. J. Clin. Nutr. 89:980S.
5. Lee, M-J. and S.K. Fried (2009) Am. J. Physiol. Endocrinol. Metab. 296:E1230.
6. Oswal, A. and G. Yeo (2010) Obesity 18:221.
7. Ogawa, Y. et al. (1995) J. Clin. Invest. 96:1647.
8. Verploegen, S.A.B.W. et al. (1997) FEBS Lett. 405:237.
9. Satoh, N. et al. (1997) Neurosci. Lett. 224:149.
10. Leroy, P. et al. (1996) J. Biol. Chem. 271:2365.
11. Savino, F. et al. (2010) Eur. J. Clin. Nutr. Jun 30 [Epub ahead of print].
12. Cohen, B. et al. (1996) Science 274:1185.
13. Tartaglia, L.A. et al. (1995) Cell 83:1263.
14. Murakami, T. et al. (1997) Biochem. Biophys. Res. Commun. 231:26.
15. Bacart, J. et al. (2010) FEBS Lett. 584:2213.
16. Tu, H. et al. (2007) J. Cell. Physiol. 212:215.

**For Research Use Only**